DELUXE FOLDING ALUMINIUM ZT-600-710 WHEELCHAIR

USER MANUAL

CE

Available Models:

ZT-600-710-SP16 (Self-Propelled with 41cm seat width)
ZT-600-710-SP18 (Self-Propelled with 46cm seat width)
ZT-600-710-TR16 (Transit with 41cm seat width)
ZT-600-710-TR18 (Transit with 46cm seat width)

Transit

Self-propelled

- 1. Maximum weight capacity 120KG
- 2. Seat width 41cm and 46cm
- 3. Frame colour silver
- 4. Upholstery colour black
- 5. Seat cushion attached to seat with Velcro strips
- 6. Both heel strap and calf strap on footrests
- 7. 41cm solid rear wheels
- 8. Storage pocket in back upholstery
- 9. Seat Belt
- 10. Half folding backrest

- 1. Maximum weight capacity 120KG
- 2. Seat width 41cm and 46cm
- 3. Frame colour silver
- 4. Upholstery colour black
- 5. Seat cushion attached to seat with Velcro strips
- 6. Both heel strap and calf strap on footrests
- 7. Quick Release 56cm solid rear wheels
- 8. Storage pocket in back upholstery
- 9. Seat belt
- 10. Half folding backrest

Please ensure that this manual is read and understood before using the wheelchair

Z-Tec Mobility
Unit 1B Albion Works, Moor Street, Brierley Hill, West Midlands DY5 3SZ

Introduction

These wheelchairs have been designed for persons with limited or no personal mobility for transport only.

This user's manual is compiled from the latest specifications and product information available at the time of publication. We reserve the right to make changes as they become necessary. Any changes to our products may cause slight variations between the illustrations and explanations in this manual and the product you have purchased.

Safety Tips

- The engineering and construction of this wheelchair have been designed to provide maximum safety.
- International safety standards currently in force have either been fulfilled or exceeded. Nevertheless users may put themselves at risk by improperly using their wheelchairs.
- The wheelchair is designed to be used by a single person only.
- For your own safety the following guidelines must be observed.
- Unprofessional or incorrect adaptation or adjustment work could increase the risk of accidents.
- Be careful during your first ride in this wheelchair.
- Get to know your wheelchair.
- Practice using your wheelchair on level ground as well as going up and down hill.
- DO NOT attempt to reach objects if you have to pick them up from the floor by reaching down between your knees.
- DO NOT attempt to reach objects if you have to move forward in the seat.
- DO NOT operate on roads or highways.
- DO NOT operate on an incline if covered in ice or a film of water or oil.
- DO NOT use the footplate as a platform when getting in or out of the wheelchair.
- DO NOT stand on the frame of the wheelchair.

SAFETY TIPS

Regular checks before use

Please check the following before each use:

- Quick release axles on the rear wheels
- Tyres and brakes. Brakes will not function properly if the tyres are worn or damaged, or if the gap between the tyre and brake is too big.
- The maximum user weight is 120kg. The wheelchair should be used exclusively to transport one person at a time in the seat. Any other use beyond this limit is in violation of safety regulations.
- Users should not sit in the wheelchair whilst riding in any means of transport.

Parts Description

Self-propelled model shown

41cm & 46cm Seat widths
Flip up Armrest
Attendant Handbrake
Swing away Footrest release lever
Parking Brake
Flip-up Footplate
Quick Release 56cm rear wheel with solid tyres (Self-propelled) & Fixed 41cm rear wheels with solid tyres (Transit)
Cross brace
Solid front castors

Handling

Opening and Folding

Opening

1. Rest both hands on each of the seat upholstery support rails and press down until the seat and back upholsteries become tight. (see photo 1)
2. Make sure that the seat support rails are safely located in the support cups.

Warning!
Do not place your fingers between the seat upholstery and the seat tubes when opening or folding the frame.

Folding

1. Lift up the footplates
2. Grasp the centre of the seat upholstery from the back and front and lift the seat upwards. This will cause the chair to fold up by its own weight.

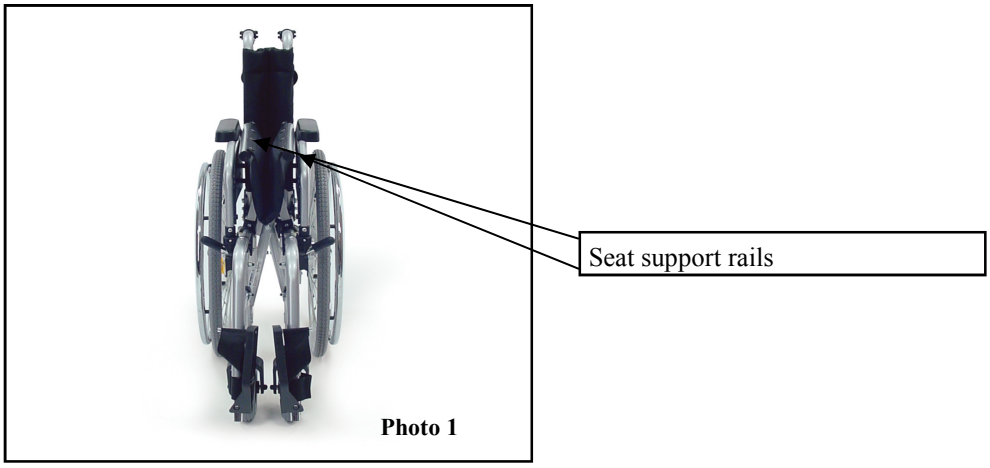

Photo 1

Folding Backrest

1. Press the release lever on each side of the wheelchair back.
2. When released fold down for easier storage,
3. Make sure the locking mechanism is fully engaged before sitting in wheelchair.

Assembly

Leg rest Assembly

Leg rest 1

- To Assemble

To fit the footrests place the top pin into the wheelchair frame. Turn the footrest assembly towards the centre of the chair and push down to secure.

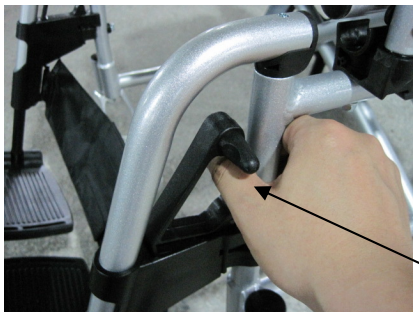

Leg rest 2

- To Remove

Pull the release lever to release the footrest assembly and either swing the assembly inwards or outwards away from the wheelchair. In this position the whole footrest assembly can be lifted and removed from the wheelchair.

Leg rest Adjustment -
For optimum comfort it is important to attain the correct leg position. The footrests have been designed so that they can be extended by
releasing the bolt on the front of the footrest hanger. This lengthens the leg rests and once a comfortable position is found the bolt should be fitted into the appropriate hole and secured tightly.

Flip up Armrest

- To Release

Push the release lever forward and lift the armrest up. This allows for side transfer if necessary.

- To Fasten

Push the armrest in to its retaining socket until secure.

Warning!
Lock armrests by securing release latch mechanism before using the wheelchair
Never lift the wheelchair by the armrests or footrests as these parts are detachable and it may cause damage to the wheelchair and/or injury to the user

Brakes

Parking Brake

The brakes are preset and adjustment should only be necessary if the brakes become loose or no longer function correctly.
To apply the parking brake push the brake lever towards the front of the wheelchair. Push the lever back to release the brakes. See photos below.
These levers are to be used by hand only.

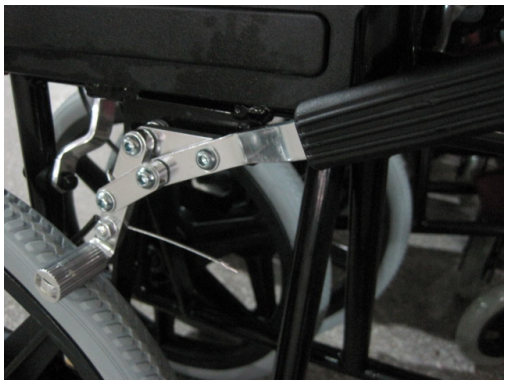

Parking Brake On

Parking Brake Off

Attendant Brake

To apply the attendant brakes squeeze the brake levers in an upward direction as shown in the photo. The running brakes are meant as an assist to the attendant. They cannot be used as a parking brake. When the wheelchair is stationary please apply both parking brakes.

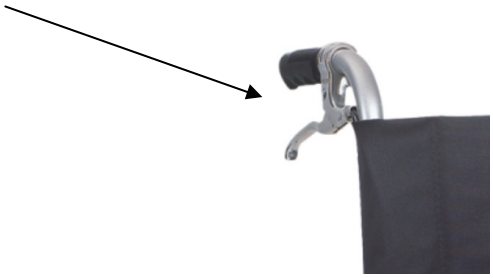

Quick Release Rear Wheel (Self-Propelled Only)

Quick Release Button

To remove the rear wheels depress the quick release button and pull the wheel away from the frame of the wheelchair. For safety reasons this should only be carried out when the wheelchair is unoccupied

Warnings

Do not stand or put pressure on the footrests when entering or exiting the wheelchair.

Should any defects become apparent on your wheelchair or if the brakes do not respond as well as expected cease using the wheelchair immediately and return it to your Z-Tec mobility dealer for inspection.
Check the tightness of the screw and bolt connections monthly.
If any connections become loose stop using the wheelchair and consult your Z-Tec mobility dealer for assistance.

Check the moving parts (e.g. wheels and leg rests) before every use.
Check that the front castors swivel freely. Withdraw from use if they do not work.
Care should be taken when assembling or dismantling the wheelchair. This wheelchair weighs (Self-propelled) 13.7kgs and (Transit) 13.9kg and care should be taken when lifting or moving it.
The wheelchair should be cleaned when necessary with a soft cloth and mild detergent.
It is recommended that you have your wheelchair serviced every 12 months, or more frequently if it is in regular use.
If the upholstery becomes worn or damaged replace it immediately.
Do not carry out unauthorised modifications to the wheelchair. Always consult your authorised dealer. Only use approved accessories as specified by Z-Tec Mobility.
Users should not sit in the wheelchair whilst travelling in any means of transport.

Warranty

Z-Tec wheelchairs are guaranteed for 12 months from the date of purchase, this warranty is not transferable. Should any part of the wheelchair require repair or full replacement as a result of a manufacturing or material defect within the warranty period, parts will be supplied free of charge. The guarantee excludes tyres and all items that have been subjected to undue wear and misuse. Under normal circumstances no responsibility will be accepted where the wheelchair has not been maintained in accordance with the manufacturer's recommendations. This does not affect your statutory rights.

If any other issues arise that are not mentioned in this user manual please write to the address on the front of this manual.